

# MODEL Q46UV MONITOR



## UV-254 and Turbidity Measurement in one sensor

Water quality monitoring continues to grow in importance as water sources come under increasing pressure. Conventional measurements of turbidity, pH, conductivity, and color provide useful information but do not reflect changes in dissolved organic constituents. Many of these dissolved organic compounds absorb UV energy. A UV-254 absorption measurement has increasingly become a useful indicator of organic carbon content, providing operators with real-time information on contaminant levels.



# MODEL Q46UV MONITOR


ATI's Model Q46UV Monitor continuously monitors the quality of raw water, treated water, recycle water, or wastewater effluents. With a relatively long 20 mm absorption path length, this sensor provides excellent sensitivity to small changes in Dissolved Organic Carbon (DOC). Employing a pulsed UV LED light source and scratch resistant sapphire optical windows, the UV-254 sensor will provide years of trouble-free monitoring.

## UV ABSORPTION & TURBIDITY IN A SINGLE SENSOR

- Long life Pulsed UV LED for extended service life.
- 20 mm measurement path for high sensitivity
- 860 nm IR turbidity measurement (ISO-7027)
- IR sensor measures both 90° scatter and absorption
- Analog outputs for both UVA and Turbidity
- Available 3rd output for DOC
- User editable table for UVA vs DOC/TOC/COD/BOD
- Chemical cleaning system option
- Automatic Sensor Fouling Compensation



## DISSOLVED ORGANIC CARBON

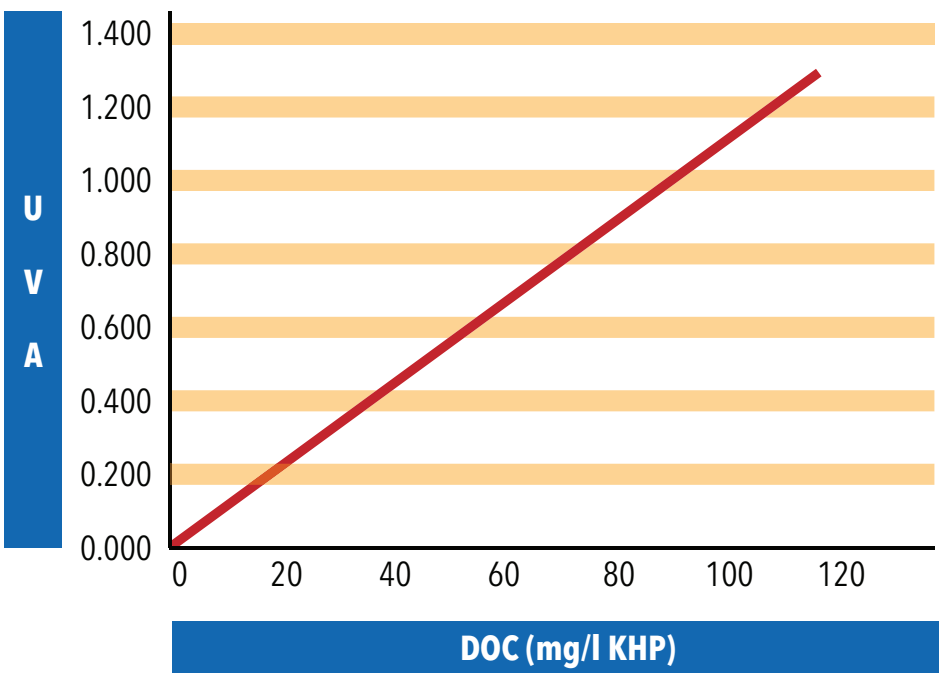


UV-254 measurements are a practical indicator of dissolved organic compounds in water. Traditional methods such as TOC, COD, and BOD all capture more organics and other potential contaminants but have the drawback of being expensive and maintenance intensive. In fact, most are done only in the laboratory due to the complexity of on-line systems.

UV-254 measurement is much simpler and can be correlated to DOC levels. It has the advantage of being nearly real time, providing input to treatment control systems and alarming of abnormal conditions. Routine maintenance consists of cleaning the optical surfaces, which is generally simple and quick.

## UV & TURBIDITY OPTICS

The Q46UV sensor provides additional optical measurements for added measurement capabilities and increased reliability. Infrared sensors for measuring both **90° Scatter Turbidity** and IR absorption are built into the UVA sensor. These additional optics allow for the measurement of **both UV-254 and Turbidity**, a unique capability to enhance the usefulness of the monitoring package, especially in raw water monitoring applications. The IR absorption measurement is used to correct measurements for minor optical fouling that can occur over weeks or months of operation.

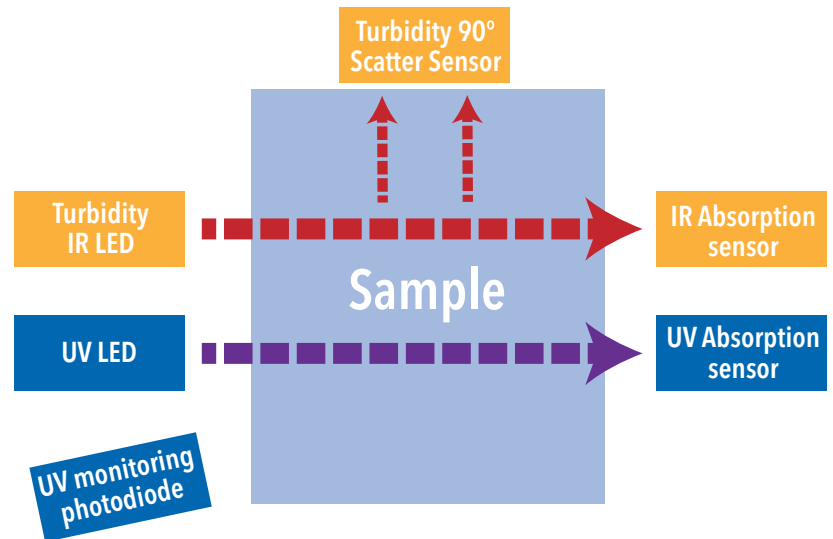


## AUTOMATIC SENSOR CLEANING

Sensors in contact with raw or settled water samples may experience fouling from iron and manganese. Prechlorination causes iron and manganese to precipitate out of solution and coat surfaces that are in contact with the sample. While manual sensor cleaning is easy, ATI offers **Q-Clean**, an automatic sensor cleaning system that reduces user maintenance.

The cleaning system consists of an automatic sensor wash system that injects a cleaning solution into the sensor flow chamber at the frequency programmed by the operator. The cleaning solution contains chemicals that dissolve iron and manganese that has accumulated on optical surfaces. The duration of the cleaning cycle is about 15 minutes but can be changed by the operator to meet specific application requirements.

## FLOWCELL OR SUBMERSIBLE INSTALLATION

UV-254 sensors are designed for either submersion or flowcell installation. Flowcells are supplied with a flow regulator installed in the outlet fitting to maintain flow at 450 ml/min.

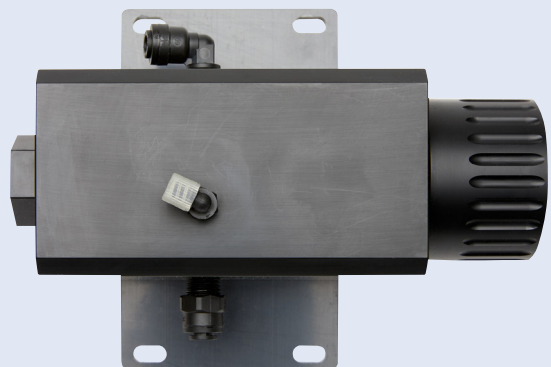

# SPECIFICATIONS

<b>Measurements /Range</b>	UVA (0-1.3 ABS), UVT (0-100%) and SUVA Surrogate measurements DOC, TOC, BOD, COD Turbidity, 0-4000 NTU, IR, 90° Scatter per ISO-7027
<b>Accuracy</b>	±0.5% UVT
<b>Repeatability</b>	±0.05% UVT
<b>Wetted Materials</b>	Anodized Aluminum Sensor (20 mm optical path), PVC flowcell
<b>Response Time</b>	90% in 3 minutes
<b>Power</b>	100-240 VAC, 50/60 Hz., 10 VA Max., 24 VDC optional
<b>Cleaning</b>	Manual cleaning standard Optional Q-Clean cleaner system available
<b>Optical Sources</b>	254 nm UV LED and Narrow 254 nm filter photodiode 780 nm IR LED for Turbidity
<b>Dimensions</b>	Probe Diameter 1.54" (39 mm), Length 6.3" (160 mm) Controller: 5.6" x 4.9" x 6.6" (142 x 125 x 168 mm)
<b>Display</b>	4 digit, 0.75" numeric LCD, 12 character second line, LED back light.
<b>Sensor Temp. Limits</b>	2° to 45°C (Operating); -40° to 70°C (Storage)
<b>Readout Temp. Limits</b>	-25° to 60°C (Operating); -40° to 70°C (Storage)
<b>Enclosure Rating</b>	Probe NEMA 6P (IP68), Control Unit NEMA 4X (IP66)
<b>Analog Output</b>	Two 4-20 mA DC, 500 ohms Max.; UVA + Turbidity, DOC, or Temp. Note: 3rd 4-20 mA output supplied if Q-Clean is not used.
<b>Relay Outputs</b>	Three SPDT alarm relays standard. Contacts rated 6 amp @ 250 VAC, 5 amp @ 24 VDC
<b>Optional Cleaner Relays</b>	Three low power relays for cleaner system control

## ORDERING INFORMATION MODEL Q46UV - A - B - C - D

### Suffix A - Power

- 1 - 100-240V +/-10%, 50/60 Hz
- 2 - 12-24 VDC, (requires 300 mA, 600 mA with Q-Clean)

### Suffix B - Sensor Type

- 1 - Submersible Sensor with 25 ft. cable
- 2 - Sensor with flowcell
- 3 - Sensor with flowcell and Q-Clean Assembly

### Suffix C - Optional Output

- 1 - 3rd 4-20 mA output
- 2 - Low power relay board (required with option B3 above)

### Suffix D - Digital output

- 1 - None
- 2 - Profibus DP
- 3 - Modbus RTU
- 4 - Ethernet/IP
- 5 - Modbus TCP/IP

### OPTIONS

- 00-1690 - Sensor Submersion mounting bracket kit
- 00-1689 - 1" Mounting Adapter for standard sensor
- 07-0100 - Universal Junction Box, NEMA 4X
- 31-0185 - 4-Conductor Interconnect Cable, specify length, max. 500 ft.
- 05-0094 - Panel mount bracket kit
- 47-0005 - 2" U-bolt, 304SS

Visit Us on the Web: [www.analyticaltechnology.com](http://www.analyticaltechnology.com)

**Analytical Technology, Inc.**  
6 Iron Bridge Drive  
Collegeville, PA 19426  
**Phone** 610.917.0991  
**Toll-Free** 800.959.0299  
**Fax** 610.917.0992  
**Email** sales@analyticaltechnology.com

**Analytical Technology**  
Unit 1 & 2 - Gatehead Business Park  
Delph New Road, Delph  
Saddleworth OL3 5DE  
**Phone** 01457 873 318  
**Fax** 01457 874 468  
**Email** sales@atiuk.com

**Represented by:**